



# Peroxidase Microplate Assay Kit User Manual

Catalog # FTA0061

(Version 1.1D)

Detection and Quantification of Peroxidase (POD) Activity in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.



I. INTRODUCTION	2
II. KIT COMPONENTS	3
III. MATERIALS REQUIRED BUT NOT PROVIDED	3
IV. SAMPLE PREPARATION	4
V. ASSAY PROCEDURE	5
VI. CALCULATION	6
VII. TYPICAL DATA	7
VIII. TECHNICAL SUPPORT	7
IX. NOTES	7



#### I. INTRODUCTION

Peroxidase (EC 1.11.1.7) is an enzyme found broadly in biological systems that utilizes hydrogen peroxide in the oxidation of various substrates. Peroxidases catalyze oxidation-reduction reactions and play an important role in protecting cell from oxidative injury.

The assay is initiated with the enzymatic catalysis of H2O2 by POD. The enzyme catalysed reaction products can be measured at a colorimetric readout at 470 nm.



#### **II. KIT COMPONENTS**

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Reaction Buffer	5 ml x 1	4 °C
Substrate	10 ml x 1	4 °C, keep in dark
Dye Reagent	4 ml x 1	4 °C
Positive Control	Powder x 1	-20 °C
Technical Manual	1 Manual	

# Note:

Positive Control: add 1 ml distilled water to dissolve before use, then take 30  $\mu$ l positive control solution into 970  $\mu$ l distilled water, mix.

# III. MATERIALS REQUIRED BUT NOT PROVIDED

- 1. Microplate reader to read absorbance at 470 nm
- 2. Distilled water
- 3. Pipettor, multi-channel pipettor
- 4. Pipette tips
- 5. Mortar
- 6. Centrifuge
- 7. Timer
- 8. Ice



#### IV. SAMPLE PREPARATION

#### 1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for  $5 \times 10^6$  cell or bacteria, sonicate (with power 20%, sonication 3s, intervation 10s, repeat 30 times); centrifuged at 8000g 4 °C for 20 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

# 2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8000g 4 °C for 20 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

# 3. For serum or plasma samples

Detect directly.



# V. ASSAY PROCEDURE

second.

Warm the Substrate, Dye Reagent to room temperature before use.

Add following reagents into the microplate:

Reagent	Sample	Positive Control	
Sample	10 μΙ		
Positive Control		10 μΙ	
Reaction Buffer	50 μΙ	50 μΙ	
Substrate	100 μΙ	100 μΙ	
Dye Reagent	40 μΙ	40 μΙ	
Mix, measured at 470 nm and record the absorbance of 20th second and 140th			

E



#### VI. CALCULATION

**Unit Definition:** one unit is defined as the OD value changed 0.01 per minute in the reaction system.

1. According to the protein concentration of sample

POD (U/mg) = (OD<sub>Sample(140S)</sub> - OD<sub>Sample(20S)</sub>) × V<sub>Total</sub> / (V<sub>Sample</sub> × C<sub>Protein</sub>) / T / 0.01  
= 
$$1000 \times (OD_{Sample(140S)} - OD_{Sample(20S)})$$
 / C<sub>Protein</sub>

2. According to the weight of sample

POD (U/g) = 
$$(OD_{Sample(140S)} - OD_{Sample(20S)}) \times V_{Total} / (W \times V_{Sample} / V_{Assay}) / T / 0.01$$
  
=  $1000 \times (OD_{Sample(140S)} - OD_{Sample(20S)}) / W$ 

3. According to the quantity of cells or bacteria

POD (U/10<sup>4</sup>) = (OD<sub>Sample(140S)</sub> - OD <sub>Sample(20S)</sub>) × V<sub>Total</sub> / (N × V<sub>Sample</sub> / V<sub>Assay</sub>) / T / 0.01  
= 
$$1000 \times (OD_{Sample(140S)} - OD_{Sample(20S)})$$
 / N

4. According to the volume of serum or plasma

POD (U/ml) = (OD<sub>Sample(140S)</sub> - OD <sub>Sample(20S)</sub>) × 
$$V_{Total}$$
 /  $V_{Sample}$  / T / 0.01  
= 1000 × (OD<sub>Sample(140S)</sub> - OD <sub>Sample(20S)</sub>)

C<sub>Protein</sub>: the protein concentration, mg/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria,  $N \times 10^4$ ;

V<sub>Total</sub>: the total volume of the enzymatic reaction, 0.2 ml;


V<sub>Sample</sub>: the volume of sample, 0.01 ml;

 $V_{\mbox{\scriptsize Assay}}$ : the volume of Assay buffer in sample preparation, 1 ml;

T: the reaction time, 2 minutes.



# VII. TYPICAL DATA

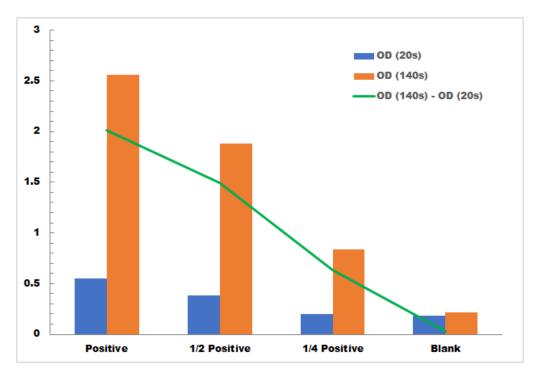

Positive Control reaction in 96-well plate assay with decreasing the concentration

#### VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.cohesionbio.com or contact us at techsupport@cohesionbio.com

#### IX. NOTES