



# **Alcohol Dehydrogenase Microplate Assay Kit User Manual**

**Catalog # FTA0083**

(Version 1.2D)

Detection and Quantification of Alcohol Dehydrogenase (ADH)  
Activity in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell  
culture media and Other biological fluids Samples.

**For research use only. Not for diagnostic or therapeutic procedures.**

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	3
IV. SAMPLE PREPARATION.....	4
V. ASSAY PROCEDURE.....	5
VI. CALCULATION.....	6
VII. TYPICAL DATA.....	7
VIII. TECHNICAL SUPPORT.....	7
IX. NOTES.....	7

## I. INTRODUCTION

Alcohol dehydrogenases (ADH) are a family of enzymes that catalyzes the conversion of alcohols to aldehydes, with the concomitant reduction of NAD<sup>+</sup> to NADH. In humans, there are nine isozymes of ADH, with the majority of ADH activity occurring in the liver. ADH family members are the primary enzymes involved in alcohol detoxification. Genetic variations in ADH enzymes result in differences in ADH activity and tolerances for alcohol, and may regulate susceptibility to alcoholism.

Alcohol Dehydrogenase Microplate Assay Kit provides a simple and direct procedure for measuring alcohol dehydrogenase activity in a variety of samples. The reaction velocity is determined by the rate of absorbance at 340 nm resulting from reduction of NADH is measured.

## II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Substrate	4 ml x 1	4 °C
Coenzyme	Powder x 1	-20 °C
Reaction Buffer	15 ml x 1	4 °C
Standard	Powder x 1	-20 °C
Positive Control	Powder x 1	-20 °C
Technical Manual	1 Manual	

### Note:

**Coenzyme:** add 1 ml distilled water to dissolve before use.

**Standard:** add 1 ml distilled water to dissolve before use; then add 0.2 ml into 0.8 ml distilled water, the concentration will be 400 µmol/L.

**Positive Control:** add 1 ml Assay Buffer to dissolve before use.

## III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 340 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice

#### IV. SAMPLE PREPARATION

##### 1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for  $5 \times 10^6$  cell or bacteria, sonicate (with power 20%, sonication 3s, interval 10s, repeat 30 times); centrifuged at 16,000g 4 °C for 20 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

##### 2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 16,000g 4 °C for 20 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

##### 3. For serum or plasma samples

Detect directly.

## V. ASSAY PROCEDURE

Warm all reagents to room temperature before use.

Add following reagents into the microplate:

Reagent	Sample	Standard	Blank	Positive Control
Standard	--	200 µl	--	
Distilled water	--	--	200 µl	
Reaction Buffer	140 µl	--	--	140 µl
Coenzyme	10 µl	--	--	10 µl
Sample	10 µl	--	--	--
Positive Control	--	--	--	10 µl
Mix, wait for 2 minutes.				
Substrate	40 µl	--	--	40 µl
Mix, measured at 340 nm and record the absorbance of 10th second and 130th second.				

### Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range. If the enzyme activity is lower, please add more sample into the reaction system; or increase the reaction time; if the enzyme activity is higher, please dilute the sample, or decrease the reaction time.

## VI. CALCULATION

**Unit Definition:** One unit of ADH activity is the enzyme that produces 1 nmol of NADH per minute.

### 1. According to the protein concentration of sample

$$\begin{aligned} \text{ADH (U/mg)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \\ &\quad / (V_{\text{Sample}} \times C_{\text{Protein}}) / T \\ &= 4000 \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}} \end{aligned}$$

### 2. According to the weight of sample

$$\begin{aligned} \text{ADH (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &\quad (V_{\text{Sample}} \times W / V_{\text{Assay}}) / T \\ &= 4000 \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

### 3. According to the quantity of cells or bacteria

$$\begin{aligned} \text{ADH (U/10}^4\text{)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \\ &\quad / (V_{\text{Sample}} \times N / V_{\text{Assay}}) / T \\ &= 4000 \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N \end{aligned}$$

### 4. According to the volume of serum or plasma

$$\begin{aligned} \text{ADH (U/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &\quad V_{\text{Sample}} / T \\ &= 4000 \times (\text{OD}_{\text{Sample(130S)}} - \text{OD}_{\text{Sample(10S)}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$

$C_{\text{Standard}}$ : the standard concentration, 400  $\mu\text{mol/L}$  = 400 nmol/ml;

$V_{\text{Standard}}$ : the volume of standard, 200  $\mu\text{l}$  = 0.2 ml;

$C_{\text{Protein}}$ : the protein concentration, mg/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria,  $N \times 10^4$ ;


$V_{\text{Sample}}$ : the volume of sample, 0.01 ml;

$V_{\text{Assay}}$ : the volume of Assay buffer, 1 ml;


T: the reaction time, 2 minutes.

## VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

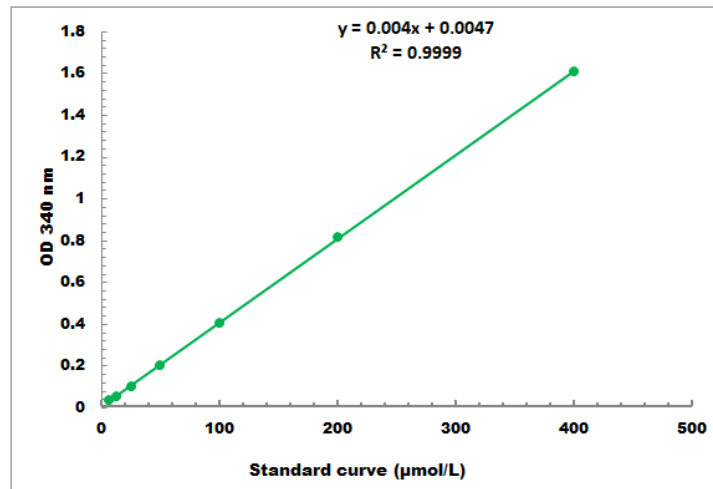

Detection Range: 4 µmol/L - 400 µmol/L

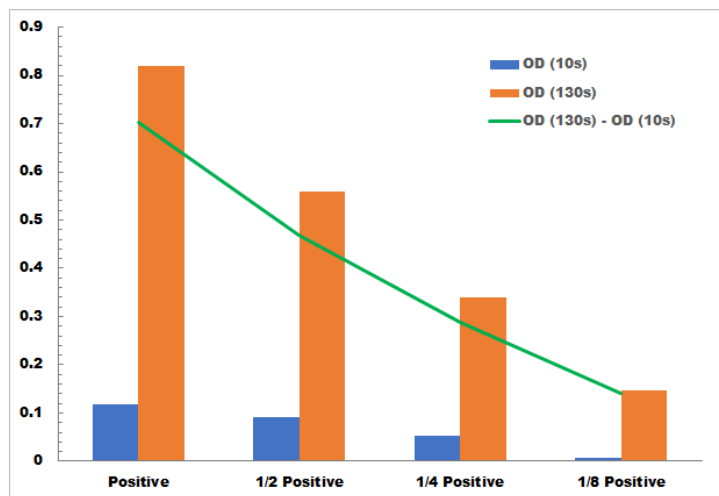

Positive Control reaction in 96-well plate assay with decreasing the concentration

## VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to [www.cohesionbio.com](http://www.cohesionbio.com) or contact us at [techsupport@cohesionbio.com](mailto:techsupport@cohesionbio.com)

## IX. NOTES