



# **Total Amino Acid Microplate Assay Kit**

## **User Manual**

**Catalog # FTA0187**

(Version 1.2A)

Detection and Quantification of Total Amino Acid Content in Urine,  
Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and  
Other biological fluids Samples.

**For research use only. Not for diagnostic or therapeutic procedures.**

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	3
IV. SAMPLE PREPARATION.....	4
V. ASSAY PROCEDURE.....	5
VI. CALCULATION.....	6
VII. TYPICAL DATA.....	7
VIII. TECHNICAL SUPPORT.....	7
IX. NOTES.....	7

## I. INTRODUCTION

Amino acids are organic compounds that contain amine and carboxyl functional groups, along with a side chain specific to each amino acid. The key elements of an amino acid are carbon, hydrogen, oxygen, and nitrogen, although other elements are found in the side chains of certain amino acids. About 500 naturally occurring amino acids are known and can be classified in many ways. They can be classified according to the core structural functional groups' locations as alpha-, beta-, gamma- or delta-amino acids; other categories relate to polarity, pH level, and side chain group type. In the form of proteins, amino acid residues form the second-largest component of human muscles and other tissues. Beyond their role as residues in proteins, amino acids participate in a number of processes such as neurotransmitter transport and biosynthesis.

Total Amino Acid Microplate Assay Kit is designed to measure total amino acid directly in biological samples without any pretreatment. The intensity of the color, measured at 570nm, is directly proportional to the total amino acid concentration in the sample.

## II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Dye Reagent	Powder x 1	4 °C
Standard	Powder x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

### Note:

**Dye Reagent:** add 10 ml distilled water heat to dissolve before use.

**Standard:** add 1 ml Assay Buffer to dissolve before use, then add 0.1 ml into 0.9 ml Assay Buffer. The concentration will be 3 mmol/L, store at 4 °C.

## III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 570 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Ice
7. Centrifuge
8. Timer
9. Convection oven

#### IV. SAMPLE PREPARATION

##### 1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for  $5 \times 10^6$  cell or bacteria, sonicate (with power 20%, sonication 3s, interval 10s, repeat 30 times); centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

##### 2. For tissue samples

Weigh 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

##### 3. For serum or plasma samples

Add 1 ml Assay buffer for 0.1 ml serum or plasma; mix; centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

## V. ASSAY PROCEDURE

Add following reagents into the microplate:

Reagent	Sample	Standard	Blank
Sample	100 µl	--	--
Standard	--	100 µl	--
Assay Buffer	--	--	100 µl
Dye Reagent	100 µl	100 µl	100 µl
Mix, put it into the convection oven, 90 °C for 20 minutes, record absorbance measured at 570 nm.			

### Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) The concentrations can vary over a wide range depending on the different samples.

For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range.

## VI. CALCULATION

1. According to the protein concentration of sample

$$\begin{aligned} \text{AA } (\mu\text{mol/mg}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &\quad (V_{\text{Sample}} \times C_{\text{Protein}}) \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}} \end{aligned}$$

2. According to the quantity of cells or bacteria

$$\begin{aligned} \text{AA } (\mu\text{mol}/10^4 \text{ cell}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &\quad (V_{\text{Sample}} \times N / V_{\text{Assay}}) \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N \end{aligned}$$

3. According to the weight of sample

$$\begin{aligned} \text{AA } (\mu\text{mol/g}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &\quad (V_{\text{Sample}} \times W / V_{\text{Assay}}) \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

4. According to the volume of sample

$$\begin{aligned} \text{AA } (\mu\text{mol/ml}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / \\ &\quad (V_{\text{Sample}} \times V / V_{\text{Assay}}) \\ &= 3 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V \end{aligned}$$

$V_{\text{Sample}}$ : the volume of the sample, 0.1 ml;

$V_{\text{Standard}}$ : the volume of the standard, 0.1 ml;

$V_{\text{Assay}}$ : the volume of Assay buffer, 1 ml;

$C_{\text{Standard}}$ : the standard concentration, 3 mmol/L = 3  $\mu\text{mol/ml}$ ;

$C_{\text{Protein}}$ : the protein concentration, mg/ml;


W: the weight of sample, g;

V: the volume of serum or plasma;

N: the quantity of cell or bacteria,  $N \times 10^4$ .

## VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

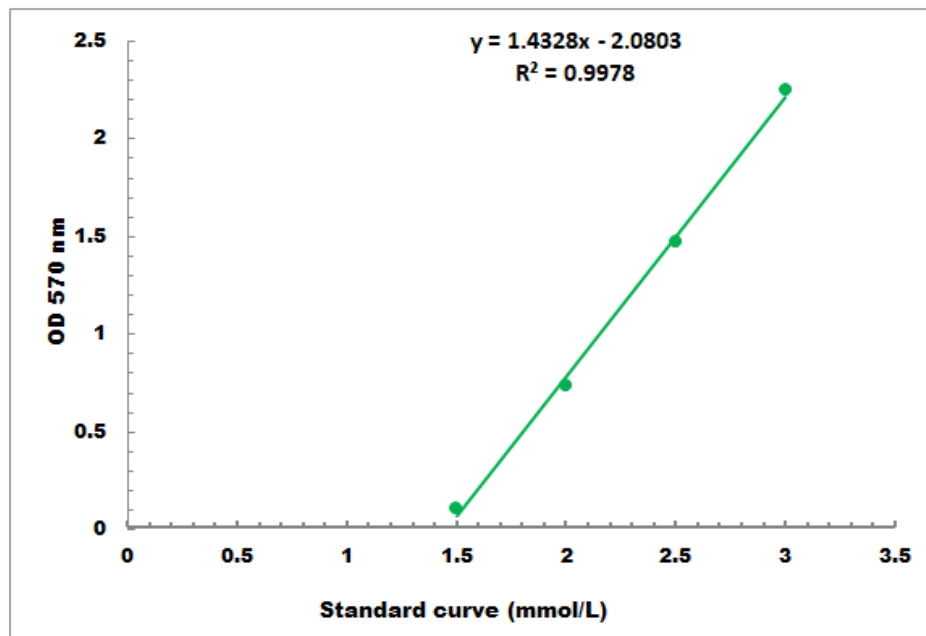

Detection Range: 1 mmol/L - 3 mmol/L

## VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to [www.cohesionbio.com](http://www.cohesionbio.com) or contact us at [techsupport@cohesionbio.com](mailto:techsupport@cohesionbio.com)

## IX. NOTES